

*FAIRCHILD PRECISION CAMERA
CALIBRATION LABORATORY*

CALIBRATION REPORT

T-11 CAMERA SERIAL NO. 51-097
INNER CONE SERIAL NO. SF288
LENS SERIAL NO. SF288

CALIBRATION CERTIFICATE

Submitted By

FAIRCHILD CAMERA AND INSTRUMENT CORPORATION
JAMAICA I, N. Y.

Camera Type T-11 Camera

Cone No. SP 268

Lens SP 283

a) Make and Type Bausch and Lomb Metrogon

b) Nominal Focal Length 6 inch

c) Maximum Aperture f/6.3

This Certificate applies to the above subject precision camera with lens as stated herein. It was tested at maximum aperture. All measurements were made with parallel light incident on the lens. The effective wave length was 575 millimicrons.

I. FOCAL LENGTH

Flange Focal Distance	Equivalent Focal Length	Calibrated Focal Length
MM	MM	MM
131.19	151.55	151.47

The probable errors of these determinations of focal length do not exceed ± 0.10 mm.

II. DISTORTION

Distortion Referred to the Calibrated Focal Length

7.5°	15°	22.5°	30°	35°	40°	45°
0.00	0.02	0.05	0.10	0.12	0.08	-0.12

The values of the distortion are measured in millimeters and indicate the displacement of the image from its distortion-free position. A positive value indicates a displacement from the center of the plate. The probable error is approximately ± 0.02 mm.

III. RESOLVING POWER (AEROGRAPHIC FILM)

	0°	7.5°	15°	22.5°	30°	35°	40°	45°
Tangential	20	26	21	21	19	20	22	12
Radial	20	22	22	22	21	20	20	19

The values of the resolving power are given at specified intervals from the center of the field and are obtained by photographing suitable test charts comprised of patterns of parallel lines. The series of patterns of the test chart are imaged on the negative with lines per millimeter spaced as follows: 10, 11, 13, 14, 16, 18, 20, 22, 25, 28, 31, 36, 40, 45, 50, 57, 63, 71, 80.

The row marked "Tangential" gives the number of lines per millimeter in the image on the negative of the finest pattern of the test chart that is distinctly resolved into separate lines when the lines lie perpendicular to the radius drawn from the center of the field. The row marked "Radial" gives similar values for the pattern of test lines lying parallel to the radius.

IV. CALIBRATION

The lines joining opposite pairs of collimation index markers intersect at an angle of $90^\circ \pm 1$ minute of arc, and their intersection indicates the location of the **point of Symmetry**, with a probable error not exceeding 0.05 mm. The ~~probable~~ ^{approximate} departure of the principal point from the auto-collimation point is ~~0.05~~ ^{0.07} mm.

V. COLLIMATION MARKER SEPARATION

A - B	237.21 mm
C - D	235.39 mm

Markers A and B lie in the line of flight.

The calibration of this camera was performed at a temperature of approximately 72° Fahrenheit.

VI. CALIBRATED FOCAL LENGTH MARKER SEPARATION

These marker separations are set at a distance equal to the calibrated focal length ± 0.05 mm.

FAIRCHILD CAMERA AND INSTRUMENT CORPORATION


PJ Morton
Precision Camera Calibration Laboratory

Jamaica, New York

Fairchild Camera and Instrument Corp.

Jamaica, New York

LeNSP 208


0.11.1.51

Cam. 51-097

Calibrated Focal Length 152.47 mm

DISTORTION IN MILLIMETERS

DISTANCE FROM P_i IN MILLIMETERS
CALIBRATED FOCAL LENGTH CURVE

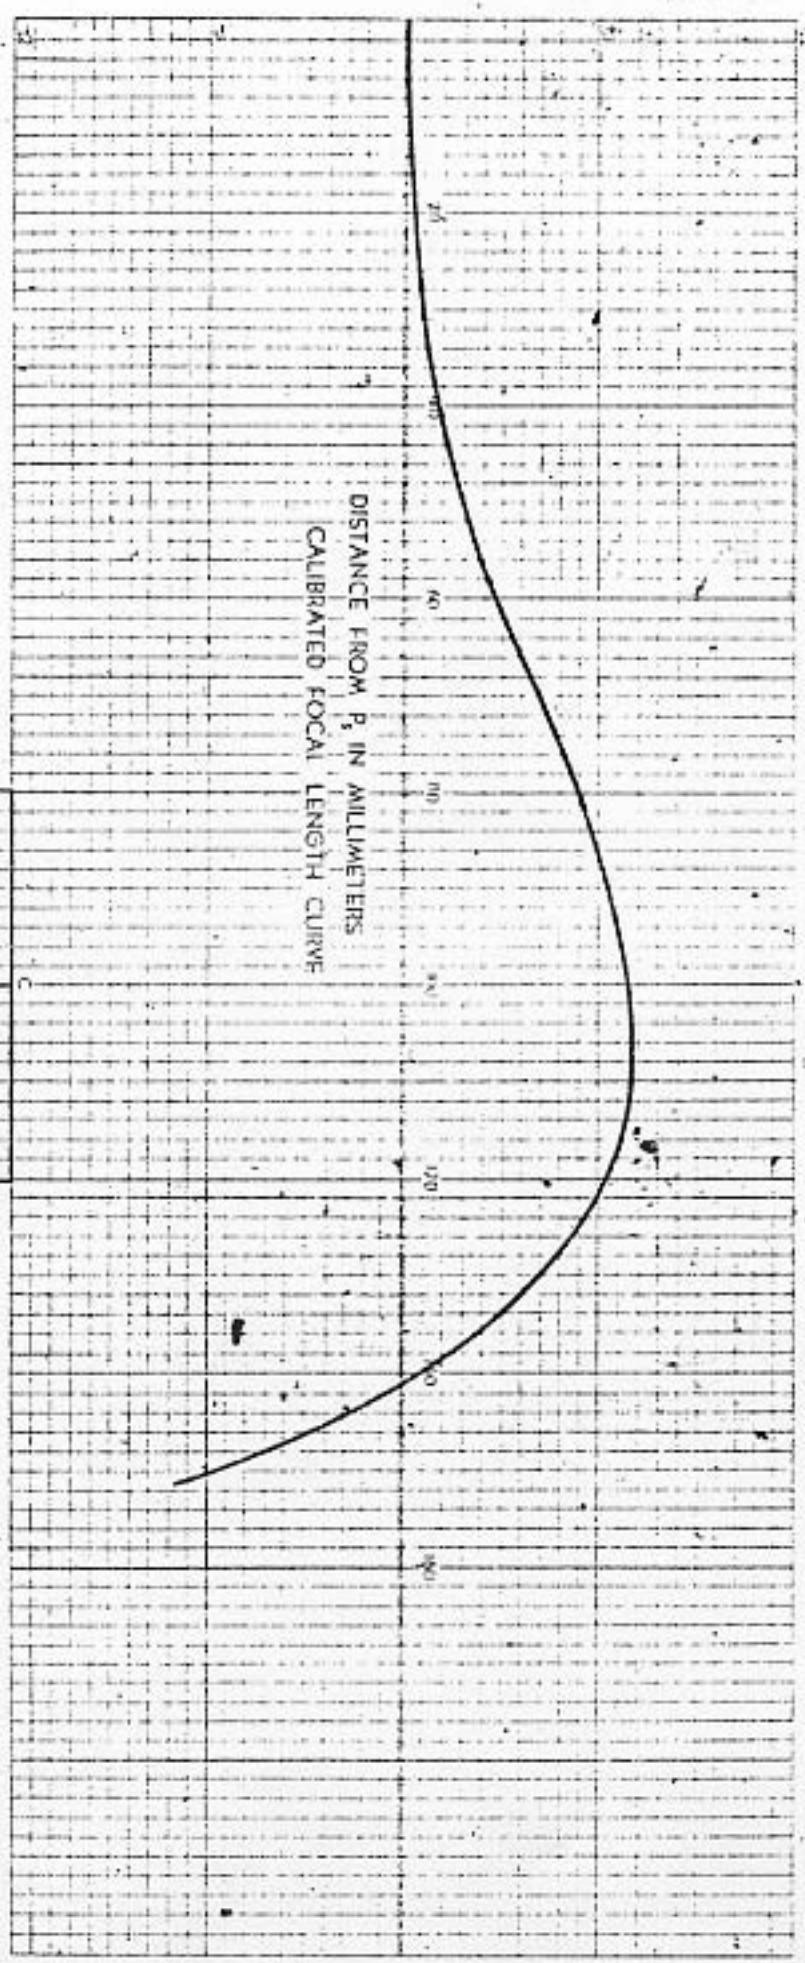

DISTANCE BETWEEN FIDUCIALS

A ————— B = 237.21 MM.
C ————— D = 35.39 MM.

$$x_{P_i} = .002 \text{ mm.}$$

$$y_{P_i} = .003 \text{ mm.}$$

RESOLUTION AEROGRAFIC FILM

Angle off Axis	Line m.m.	Line m.m.
0	20	20
7.5	26	22
15	21	22
22.5	21	22
30	19	21
35	20	20
40	22	20
45	22	20

Signed
R. M. Morton

Precision Camera Calibration Laboratory